



Tritium Laboratory  
25 September 2025

SWAB REPORT # 1130

SWAB DATE: 1 September 2025

*R/V Thomas G. Thompson*

---

Dr. James D. Happell  
Associate Research Professor

Distribution:  
SWAB Committee  
Brandi Murphy  
Sarah McCullagh  
Joyce Chambers

## COMMENTS TO SWAB REPORTS

15 December 2021

The LSC is now a Quantulus GCT 6220, with the SWAB counting assay having background cpm of 0.3 & 1.2 for  $^3\text{H}$  &  $^{14}\text{C}$ . This replaces an LSC with background cpm of 1.6 & 5.5 for  $^3\text{H}$  &  $^{14}\text{C}$ .

All samples are counted for 60 minutes, the instrument background is subtracted, and activities are reported in  $\text{dpm/m}^2$ . Bucket blank activities are not subtracted. Counting errors (2 standard deviations) are also reported in  $\text{dpm/m}^2$ . An error larger than the activity indicates that the activity is not significantly different from zero. All activities significantly above background will be in **bold**.

### Criteria for SWAB Results

Category	$^3\text{H}$ ( $\text{dpm/m}^2$ )	$^{14}\text{C}$ ( $\text{dpm m}^2$ )	Recommendations
A	<500	<50	No action
B*	500-10,000	50-10,000	Needs cleaning before any natural tracer work. Decks in radiation vans with activities above $1000 \text{ dpm/m}^2$ should be cleaned.
C**	10,000-100,000	10,000-50,000	Must be cleaned before any use.
D***	>100,000	>50,000	May be a health hazard. Notify local radiation safety official.

Note:  $^{14}\text{C}$  and  $^{35}\text{S}$  have peak energies of 156 and 167 KeV, respectively; thus  $^{35}\text{S}$  will be registered as  $^{14}\text{C}$  by our counting techniques. Categories A, B and C are not a health hazard.

### Recommended Cleaning Procedure

Wearing ordinary household rubber gloves:

$^3\text{H}$ : Wash and scrub with radioactive cleanup detergent such as COUNT-OFF (50 ml COUNT-OFF to 4 liters of water), using sponges to distribute solution and reabsorb it.

$^{14}\text{C}$ : Wash with 1% sulfuric or 2% hydrochloric (muriatic) acid with good ventilation (will dissolve carbonates, releasing  $^{14}\text{CO}_2$ ). Follow up with wash as if for  $^3\text{H}$ .

### Disposal of Cleaning Materials (gloves, sponges, etc)

Categories A & B dispose as ordinary garbage, C & D contact your institution's radiation safety office.

Note: If category C or D is encountered, we try to notify the institution promptly by phone or email.

# REPORT FOR SWAB #1130

LOCATION: Singapore

DATE: 1 September 2025

VESSEL: R/V Thomas G. Thompson

TECHNICIAN: Brandi Murphy

Sample #	Sample Identification	<sup>3</sup> H dpm/m <sup>2</sup>			<sup>14</sup> C dpm/m <sup>2</sup>		
		activity	error		activity	error	
1	1st Vial Bkgnd	0	±	0	0	±	0
2	Initial bucket blank	1	±	8	4	±	13
	<u>Main Lab (Figure 1)</u>						
3	Starboard sink area	-3	±	28	12	±	14
4	Port sink area	18	±	19	15	±	13
5	Inside fume hood	-7	±	34	-7	±	14
6	Inside GE refrigerator	-2	±	30	8	±	13
	<u>BioAnalytical Lab (Figure 2)</u>						
7	Inside fume hood	-18	±	39	16	±	14
8	Aft sink area	7	±	34	-4	±	9
9	Inside refrigerator	-17	±	36	0	±	1
	<u>Computer Lab (Figure 3)</u>						
10	Center benchtop	-62	±	63	11	±	21
	<u>Hydro Lab (Figure 4)</u>						
11	Port sink area	-30	±	48	17	±	15
12	Aft end of center bench	9	±	14	14	±	13
	<u>Wet Lab (Figure 5)</u>						
13	Sink area	-9	±	42	-9	±	18
14	Forward workbench	12	±	26	-2	±	4
	<u>Main Deck (Figure 6)</u>						
15	Deck of container bay	-16	±	34	-10	±	19
16	Stern port quarter	-37	±	59	10	±	16
17	Final bucket blank	-25	±	52	15	±	15

## Comments

Please note that the error reported for each isotope is the two-standard deviation counting error. Reports may now contain values less than zero. Decay counting background samples will be distributed about the background vial, which means that negative values are possible. In the past we rounded the negative values to zero. Values are only significantly above background when they are positive and larger than the error. Please note that we are now using a Quantulus 6220 LSC which counts very near natural background. While the cleanup standards have not changed all values above background will now be in bold. All areas tested on the ship were free from isotope contamination requiring cleaning.

## Main Lab Layout

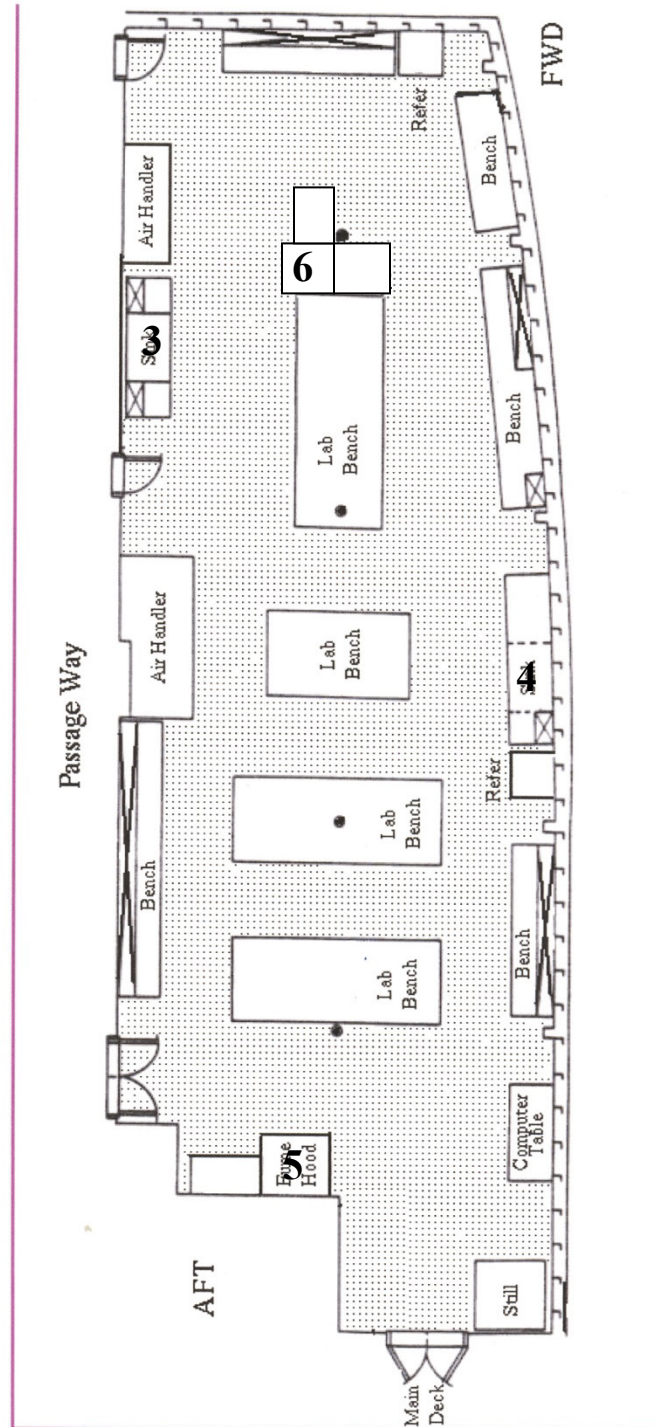


Figure 1  
SWAB 1130  
1 September 2025

Figure 2  
SWAB 1130  
1 September 2025

### BioAnalytical Lab Layout

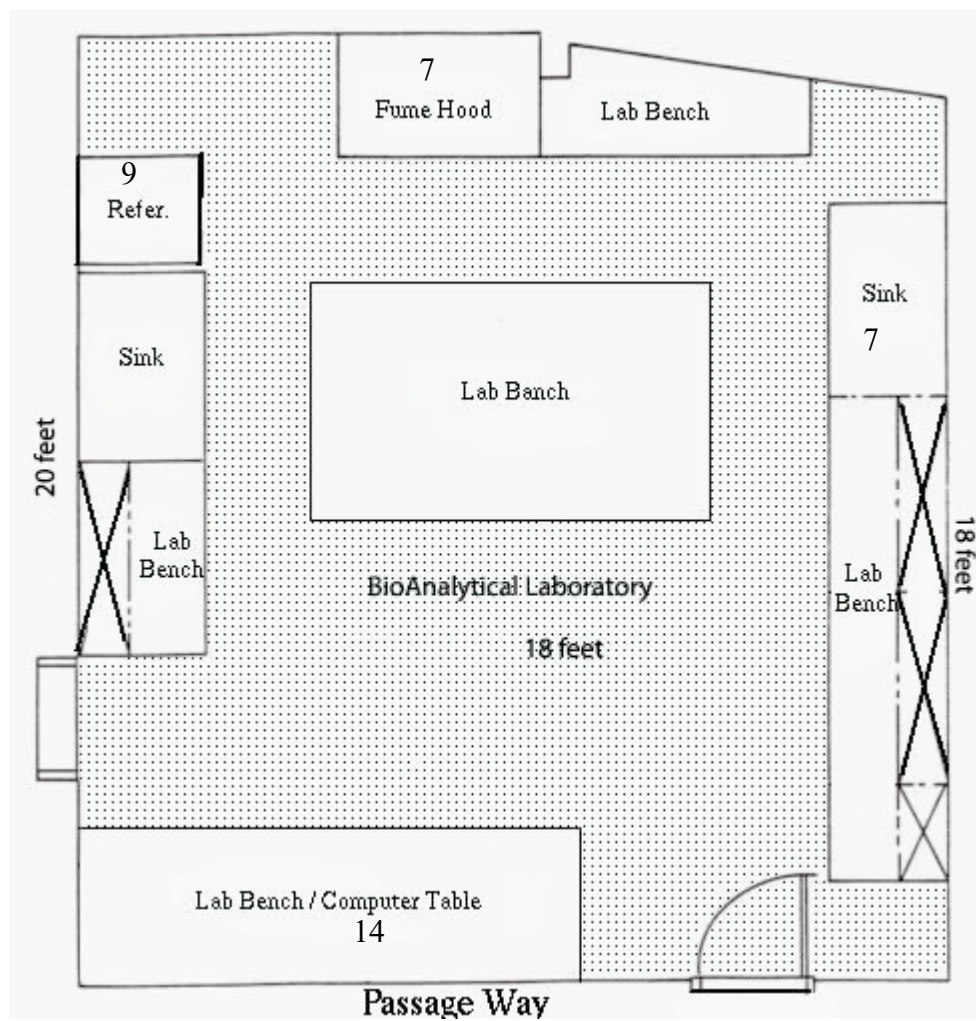


Figure 3  
SWAB 1130  
1 September 2025

### Computer Lab Layout

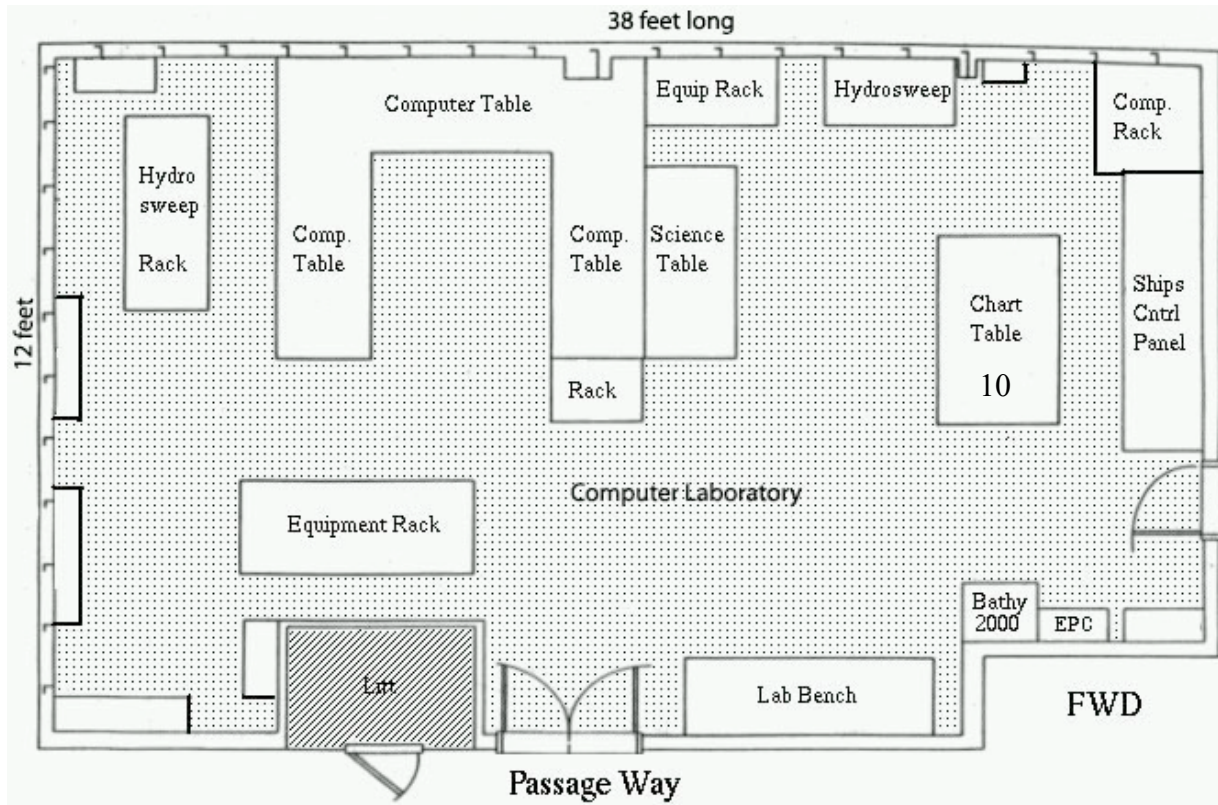


Figure 4  
SWAB 1130  
1 September 2025

## Hydro Lab Layout


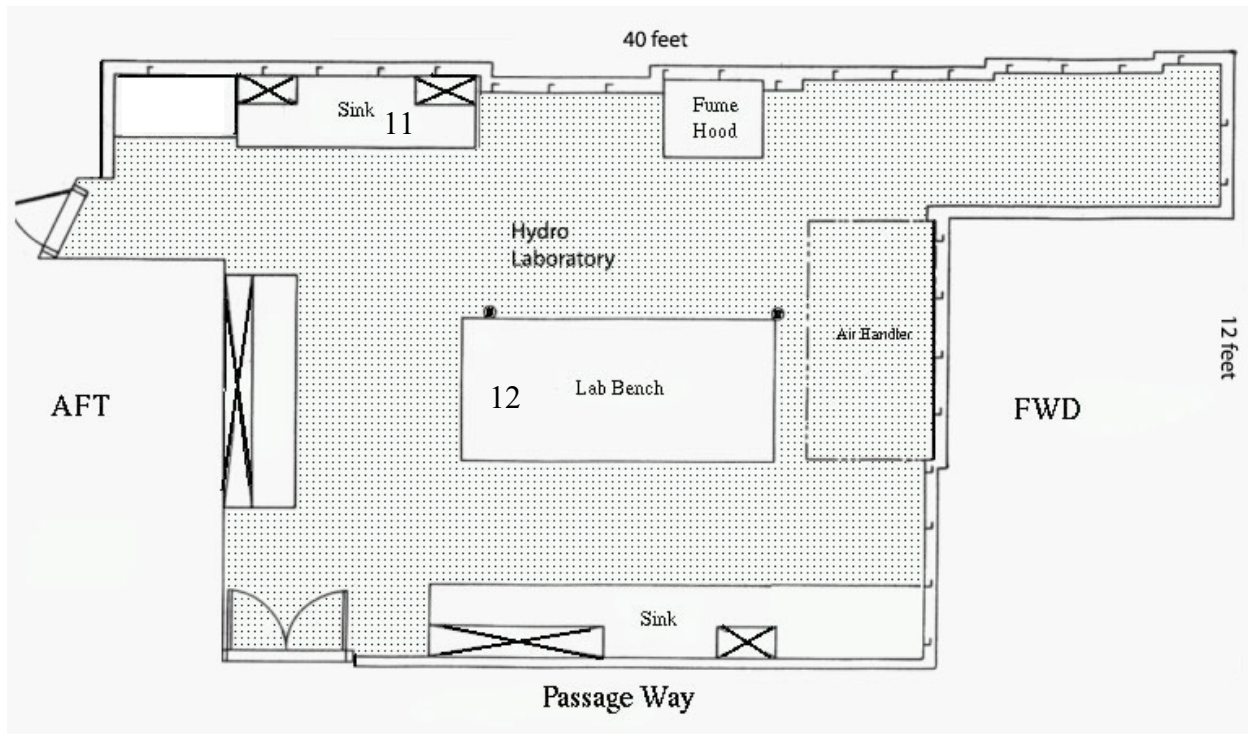




Figure 5  
SWAB 1130  
1 September 2025

Wet Lab Layout



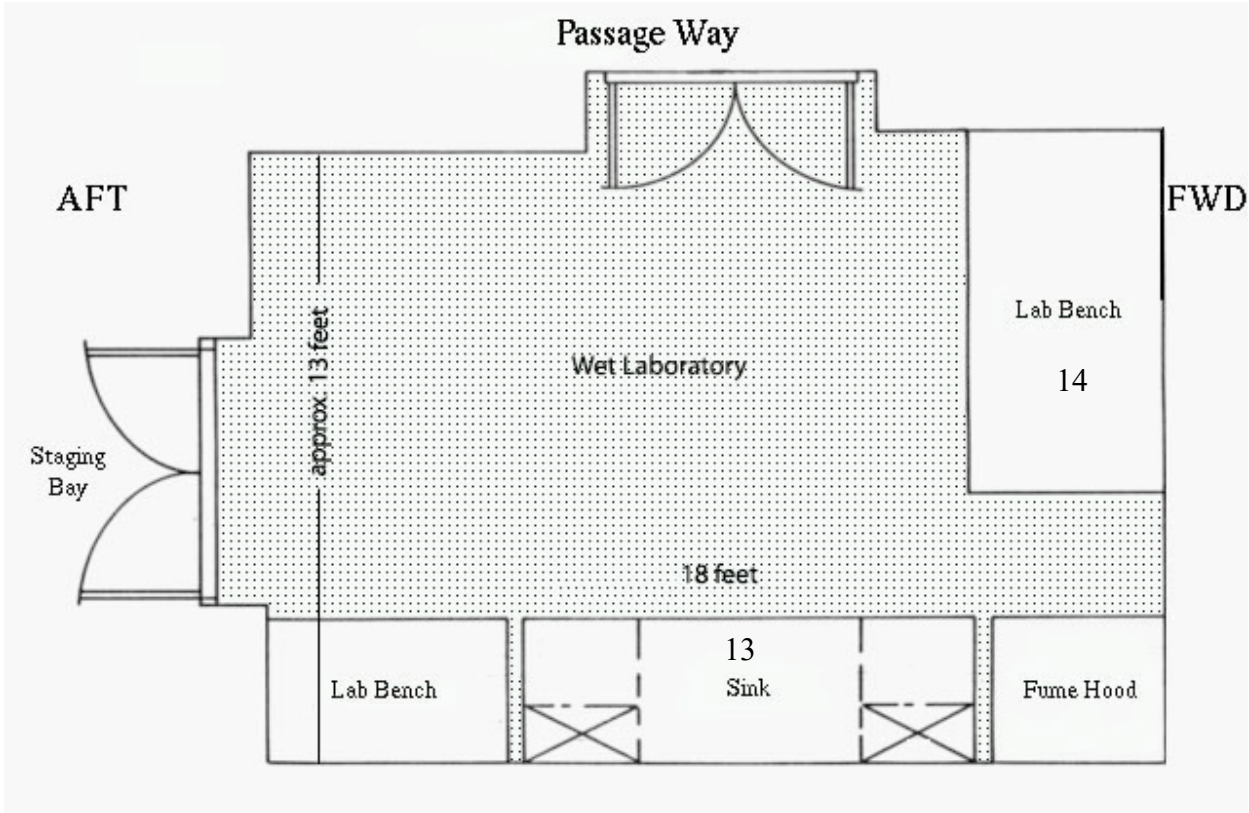

	N	Gd	A	GA
--	---	----	---	----

